

.. THE JPL **Hg+** EXTENDED LINEAR ION TRAP FREQUENCY STANDARD:  
STATUS, STABILITY, AND ACCURACY PROSPECTS\*

R. L. Tjoelker, J. D. Prestage, L. Maleki

Jet Propulsion Laboratory, California Institute of Technology  
4800 Oak Grove Drive, MS 298-100  
Pasadena, California 91109

Abstract

Microwave **frequency** standards based on room temperature  $^{199}\text{Hg}^+$  ions in a Linear Ion Trap (LITS) presently achieve a Signal to Noise and line Q inferred short term frequency stability of  $\sigma_y(\tau) = 2 \times 10^{-14}/\tau^{1/2}$ . Long term stability has been measured for averaging intervals up to 5 months with apparent sensitivity to variations in ion number/temperature limiting the flicker floor to about  $5 \times 10^{-16}$  at 100,000 seconds. A two segment version of the linear ion trap (LITE) has also recently demonstrated excellent frequency stability for measurement intervals up to one week. Nearly an order of magnitude improvement in long term stability compared to the LITS is expected since this trap **configuration** operates with reduced linear ion density during the microwave interrogation period.

INTRODUCTION

Mercury Linear Ion **Trap frequency** Standards (LITS) have been developed at JPL to address the practical needs of the NASA Deep Space Network (DSN) with the goal of providing frequency stability substantially better than the hydrogen masers currently in use in each DSN station. The DSN requires high frequency stability for communication and tracking of a variety of spacecraft throughout the solar system. The stability needs vary from less stringent requirements for navigation, to more demanding requirements for very long baseline interferometry, gravity wave searches, and radio science experiments. Most recent frequency and timing stability requirements for the upcoming **CASSINI** mission to Saturn are near  $10^{-15}$  stability from 1 to tens of thousands of seconds. Frequency standards in the DSN must provide very high stability and operate continuously at remote locations from JPL. This requires the standards to be reasonably transportable, operate autonomously, and be very reliable.

THE LINEAR ION TRAP STANDARD (LITS)

The ongoing development of the LITS [1-5] based on the 40.5 GHz ground state **hyperfine** transition of  $^{199}\text{Hg}$  ions [6] has recently led to the development of an engineering model for the DSN [7]. Ions confined in a trap allow for long interrogation times and high atomic line Q. Continuous operation is made practical using a  $^{202}\text{Hg}$  lamp to generate 194.2 nm radiation for atomic state selection and a helium buffer gas for ion cooling [8]. The large 40.5 GHz  $^2\text{S}_{1/2}(F=0, m_F=0)$  to  $^2\text{S}_{1/2}(F=1, m_F=0)$  ground state **hyperfine** transition in mercury is less susceptible to magnetic and Doppler **shifts** than in transitions in lighter atoms providing good long term frequency stability with minimal environmental regulation. The linear ion trap provides a way to increase the detected fluorescence

signal to noise (MN) without increasing the second order Doppler shift [1]. The  $^{199}\text{Hg}^+$  hyperfine transition is typically interrogated using Ramsey successive oscillatory fields with two 0.4 second microwave pulses separated by an interrogation time ranging from 1 to 30 seconds, depending on the local oscillator.

Presently achieved Signal to Noise and line Q with a LITS (Fig. 1) infer a short term frequency stability of  $\sigma_y(\tau) = 2 \times 10^{-14} \tau^{-1/2}$  [7]. A major challenge to realizing the full stability has been the stability of the local oscillator. To date, only a quartz VCXO or some hydrogen masers have had sufficient reliability to serve as LO's for trapped ion frequency standards in the DSN. In both cases the achievable frequency stability is compromised due to local oscillator frequency noise at multiples of the interrogation cycle frequency [9]. Liquid helium cooled sapphire resonator technology provides stability that is sufficient to not degrade the LITS stability. Unfortunately the need to periodically fill a helium Dewar has limited the practicality of using cryogenic sapphire as a permanent local oscillator. A program at JPL has recently been initiated to develop a continuously operating Compensated Sapphire Oscillator (CSO) cooled with a closed cycle refrigerator to  $\approx 10$  K [10]. The frequency stability goal of  $3 \times 10^{-15}$  for 1 to 100 seconds will provide an ideal local oscillator for the LITS. The CSO/LITS combination will meet all radio science and gravity wave search frequency stability needs in the DSN for the upcoming Cassini mission to Saturn. Figure 2 shows schematically the LITS short term stability when operated with a quartz VCO or a hydrogen maser as the LO. Also shown is the projected stability when operated with the CSO under development and the LITS operating at  $\sigma_y(\tau) = 2 \times 10^{-14} / \tau^{1/2}$ .

The long term stability (and potential accuracy) is fundamentally related to the size of sensitivity to environmental perturbations and the ability to know and control (measure) them. The three largest frequency offsets in present LITS operation [3] are 1) the Second Order Zeeman Shift (DC magnetic fields) 2) the 2nd Order Doppler shift (due to thermal and driven ion motion), and 3) a pressure shift due to collisions with the helium buffer gas. In the LITS, the entire trap, W optics systems, and Helmholtz coils are surrounded by five large nested magnetic shields. This magnetic shielding is sufficient to reduce external magnetic field fluctuations by 20,000 providing a fractional frequency sensitivity to external fluctuations of  $\approx 2 \times 10^{-17} / \text{mG}$ . The trap/optics/shield region requires thermal regulation to only 0.1 °C to achieve a frequency stability of  $10^{-5}$ . Long term stability requires the ion number/temperature to be stable over the length of the averaging interval. The ion number depends on several operating parameters, trap well depth, ion load and loss rate, and the condition of the vacuum. The vacuum system has a base pressure of  $\approx 1 \times 10^{-9}$  Torr, a mercury background pressure of about  $\approx 5 \times 10^{-10}$  Torr and a helium buffer gas pressure of  $\approx 10^{-8}$  Torr. Mercury vapor is generated by heating a small sample of HgO to approximately 200 °C, and helium is introduced through a heated quartz helium leak and stabilized to an ion gauge pressure measurement. Possible aging of the vacuum system, ion gauge, or changes in the Hg pressure as a function of HgO temperature over time are presently not controlled though the electron current used to ionize  $^{199}\text{Hg}$  atoms and the temperature of the HgO source are regulated. The longest continuous stability measurement to date in this "open loop" operation is a 5 month comparison between an early research standard (LITS-2) and a cavity tuned hydrogen maser [4,5]. Over this 5 month interval the relative long term drift was measured to be  $2.1(0.8) \times 10^{-16} / \text{day}$ . Stability comparisons up to one month have been performed between two LITS standards, with the flicker floor of the earliest LITS standards LITS-1 and LITS-2 measured at  $5 \times 10^{-16}$  at 100,000 seconds [5]. The source of this limit, though not

completely resolved, apparently arises from variations of the ion number/temperature as a function of vacuum parameters which change slightly under environmental perturbations.

## RECENT RESULTS WITH THE EXTENDED LINEAR ION TRAP STANDARD(LITE)

An extended version of the current LITS standards (often referred to as 'LITE' or 'Shuttle trap') provides several advantages to the current LITS scheme [11,12]. The LITE consists of two separate trap regions, a magnetically shielded region for microwave interrogation, and a separate region for ion loading and state preparation/detection using 194 nm light. Ions are "shuttled" back and forth between these two regions using only DC potentials. Practical advantages are that the LITE can be made much smaller (perhaps even for spaceflight [13,14]), more maintainable (because of improved access to lamp and photon detectors), and should offer reduced sensitivity to environmental perturbations. Performance advantages, especially towards further improvements of long term stability and accuracy should result by operating at reduced ion densities during microwave interrogation. Therefore the sensitivity to the portion of the second order Doppler shift most difficult to keep stable (i.e. ion number fluctuation in the trapping RF field) is significantly reduced without reducing signal to noise or line Q. This long term performance gain comes without further improvements to environmental regulation or compromising continuous reliable operation.

Figure 3 shows the 40.507 GHz signal resulting from Ramsey interrogation of ions in the first LITE trap, The resonant frequency measured represents the magnetically shielded hyperfine transition, though fluorescence detection actually occurred when the ions were subject to the earth's ambient magnetic field, The inferred performance in Fig.3 is  $\sigma_y(\tau) = 5.9 \times 10^{-14} / \tau^{1/2}$ , accomplished with an 11.1 second interrogation time and only a single detection system. With a second collection system a  $\sqrt{2}$  improvement would give a performance of  $4 \times 10^{-14} / \tau^{1/2}$ , already within a factor of 2 of the best ever measured in a LITS. Figure 4 shows a 5 day stability comparison using a hydrogen maser as the local oscillator and an SAO hydrogen maser[15] as the reference. The performance shown indicates good intermediate term stability between 20 and 20,000 seconds (The data shown for times less than 20 seconds is an artifact of the measurement technique). For comparison times longer than 20,000 seconds, the stability is most likely limited by drift in the maser. Longer term comparisons to a LITS have yet to be done, though it is expected that the long term stability of the LITE will be significantly better than the current LITS.

A new "shuttle" trap standard currently being developed in our laboratory solely for performance enhancements is shown in Fig. 5. Significantly improved magnetic field homogeneity should allow operation at lower magnetic fields by a factor of nearly 8 reducing sensitivity to external and applied magnetic perturbations. The extended trap will have an interrogation region 7 times longer than in the present LITS, reducing sensitivity to all long term systematic affected by ion number/temperature variations. In principle, this could reduce the flicker floor to  $\approx 1 \times 10^{-16}$  with corresponding improvements to long term stability without additional environmental regulation.

Though there is still much stability and accuracy to be gained operating at room temperature, stability performance significantly below  $10^{-16}$  will most likely require cold ions (and a superb LO). Unfortunately most ion based microwave standards require ultra-violet light for optical pumping and/or laser cooling. While single laser cooled ions may in principal provide the highest accuracies

[16].the need for stability and practical laser system currently makes the approach of direct laser cooling and detection inappropriate for the DSN. An alternative approach, which may prove to be more practical, may be the possibility of using laser cooled neutral atoms for state detection and cooling of trapped ions [14].

## CONCLUSION

A mercury linear ion trap frequency standard, has been developed for continuous operation and tested in the NASA Deep Space Network. Measured signal to noise, and atomic line Q indicate that a short term stability performance of  $\sigma_y(\tau)=2 \times 10^{-14}/\tau^{1/2}$  can be achieved when operated with an appropriate local oscillator. Recent developments in sapphire resonator fabrication has resulted in an effort at JPL to develop a continuous operating Compensated Sapphire Oscillator (CSO). This oscillator when steered with the LITS should provide frequency stability around  $10^{-15}$  from times ranging from 1 second to months.

Initial measurements taken with the first LITE (shuttle) standard show a short term stability similar to the LITS. A stability measurement for 5 days indicated that the flicker floor is at least equivalent to the LITS with significant improvements to long term stability expected. In a second generation "shuttle" trap currently under development, the flicker floor resulting from current environmental sensitivity may be reduced by a factor of seven. When operated with the CSO as a local oscillator very low flicker floors, perhaps breaking into the  $10^{-17}$  region, should be possible for averaging times less than 100,000 seconds. Longer term stability (and potential accuracy determination) should also be improved by the achievable sensitivity reduction. This would be accomplished using the same electronics as the LITS and the same low degree of environmental regulation.

---

\*This work was performed at the Jet Propulsion Laboratory, California Institute of Technology, under contract to the National Aeronautics and Space Administration.

## References

- [1] J.D. Prestage, G. J. Dick, L. Maleki, "New Ion Trap for Frequency Standard Applications", *J. Appl. Phys.* 66, No. 3, 1013-1017, August 1989.
- [2] J.D. Prestage, R.L. Tjoelker, G.J. Dick, L. Maleki, "Ultra-Stable Hg<sup>+</sup> Trapped Ion Frequency Standard", *J. Mod. Opt.* 39, No. 2, 221-232, 1992.
- [3] R.L. Tjoelker, J.D. Prestage, G.J. Dick, L. Maleki, "Long Term Stability of Hg<sup>+</sup> Trapped Ion Frequency Standards", *Proc. 47th Ann. Symp. Freq. Control*, p 132, June 1993.,
- [4] R.L. Tjoelker, J.D. Prestage, G.J. Dick, L. Maleki, "Recent Stability Comparisons With The JPL Linear Trapped Ion Frequency Standards", *Proc. 48th Ann. Symp. Freq. Control*, 739-743, June 1994.

[5] **R.L. Tjoelker, J.D. Prestage, L. Maleki**, "Record Frequency Stability with Mercury in a Linear Ion Trap", **Proc. 5th Symp. Freq. Standards and Metrology, Woods Hole MA**, 33-38, October 1995.

[6] F. G. Major and G. Werth, "Magnetic Hyperfine Spectrum of Isolated  $^{199}\text{Hg}^+$  Ions", *Appl. Phys.* 15,201-208, 1981.

[7] **R.L. Tjoelker, C. Bricker, W. Diener, R.L. Hammel, A. Kirk, P. Kuhnle, L. Maleki, J.D. Prestage, D. Santiago, D. Seidel, D.A. Stowers, RL. Sydnor, T. Tucker**, "A Mercury Ion Frequency Standard Engineering Prototype for the NASA Deep Space Network", **Proc. 50th Ann. Symp. Freq. Control**, 1073-1081, June, 1996.

[8] L. S. Cutler, R. P. Giffard, and M. D. McGuire, "Thermalization of  $^{199}\text{Hg}$  Ion Macromotion by a Light Background Gas in an RF Quadruple Trap", *Appl. Phys. B* 36, 137-142, 1985.

[9] G.J. Dick, J.D. Prestage, C.A. Greenhall, and L. Maleki, "Local Oscillator Induced Degradation of Medium-Term Stability in Passive Atomic Frequency Standards" in **Proc. 22nd Annual Precise Time and Time Interval (PTTI) Meeting**, 487-508 (1991).

[10] R. Wang, and G.J. Dick, "10 Kelvin Compensated Sapphire Resonator for Cassini Mission"; in **Proc. for the Scientific Applications of Clocks in Space Workshop, Pasadena, CA**, November 7-8, 1996

[11] J.D. Prestage, R.L. Tjoelker, G.J. Dick, and L. Maleki, "Improved Linear Ion Trap Package", **Proc. 47th Ann. Symp. Freq. Control**, p. 148, June 1993.

[12] J.D. Prestage, R.L. Tjoelker, G.J. Dick, L. Maleki, "Progress Report on the Improved Linear Ion Trap Physics Package", **Proc. 49th Ann. Symp. Freq. Control**, 82-85, June 1995.

[13] J.D. Prestage and L. Maleki, "Space flyable  $\text{Hg}^+$  Frequency Standards", **Proc. 48th Ann. Symp. Freq. Control**, 747-754, June 1994.

[14] J.D. Prestage, R.L. Tjoelker, L. Maleki, "Trapped Ion Clock for Space Applications"; in **Proc. for the Scientific Applications of Clocks in Space Workshop, Pasadena, CA**, November 7-8, 1996

[15] Smithsonian Astrophysical Observatory; Cambridge, Massachusetts 02138 USA.

[16] J.D. Miller, D.J. Berkeland, F.C. Cruz, J.C. Bergquist, W.M. Itano and D.J. Wineland, "A Laser-Microwave Double Resonance Frequency Standard Using  $^{199}\text{Hg}^+$  Ions in a Cryogenic Linear Trap", **Proc. 50th Ann. Symp. Freq. Control**, 1086-1088, June 1996,

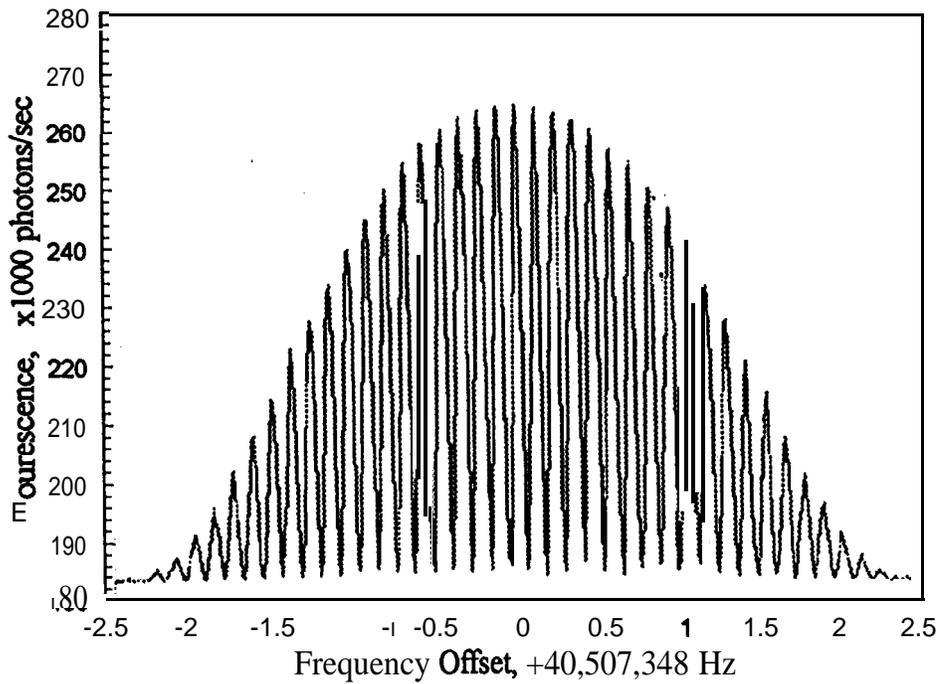


Figure 1: The 8 second Ramsey interrogation signal from the engineering prototype LITS-4 (cycle time 12 seconds). this signal to noise and line Q correspond to a stability of  $2.0 \times 10^{-14}/\tau^{1/2}$

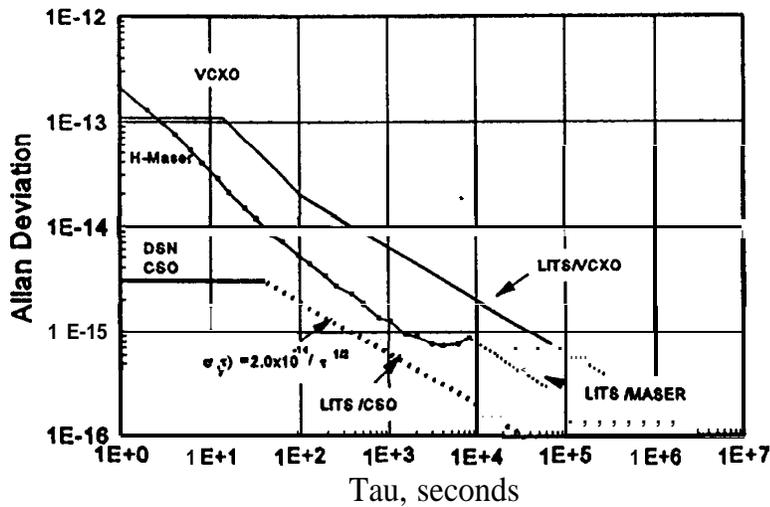


Figure 2: LITS performance shown using either a quartz VCO or a hydrogen maser as the local oscillator. Also shown is the expected performance with a continuously operating compensated sapphire oscillator under development and the LITS operating at  $2.0 \times 10^{-14}/\tau^{1/2}$ .

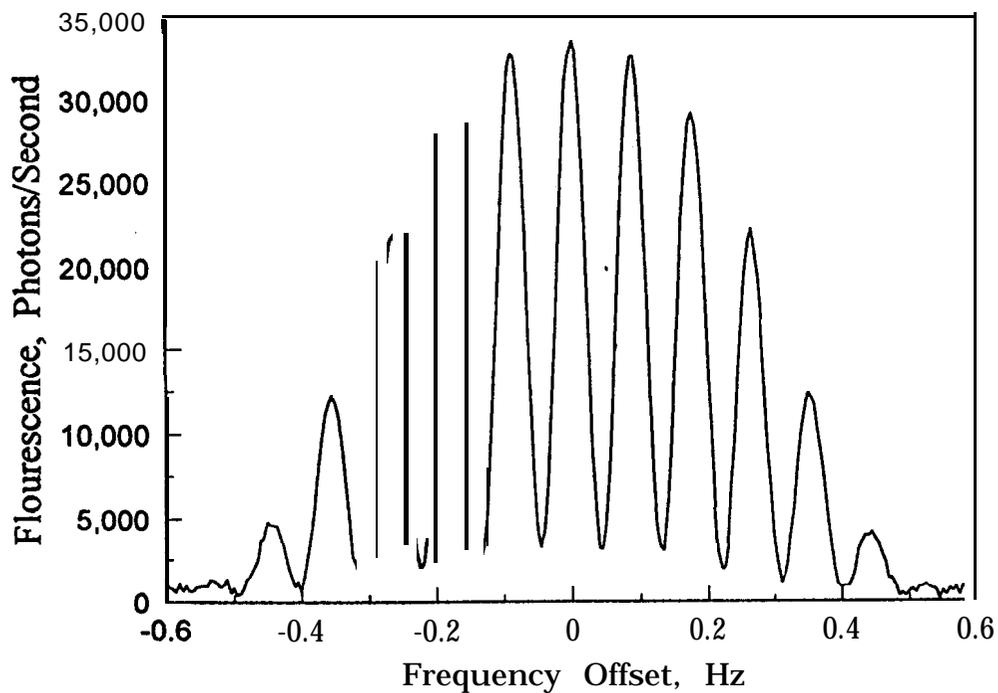


Figure 3: Ramsey interrogation tinges from 11.1 second interrogate ion cycle in the first LITE research standard.

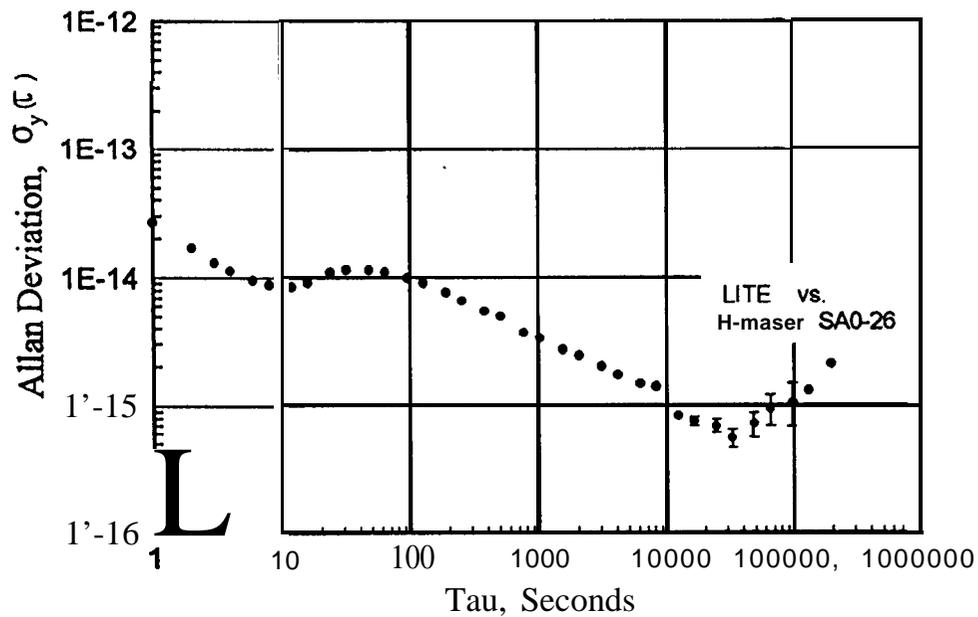


Figure 4: Five day frequency stability mmparison of the first LITE research standard to the hydrogen maser SAO-26.

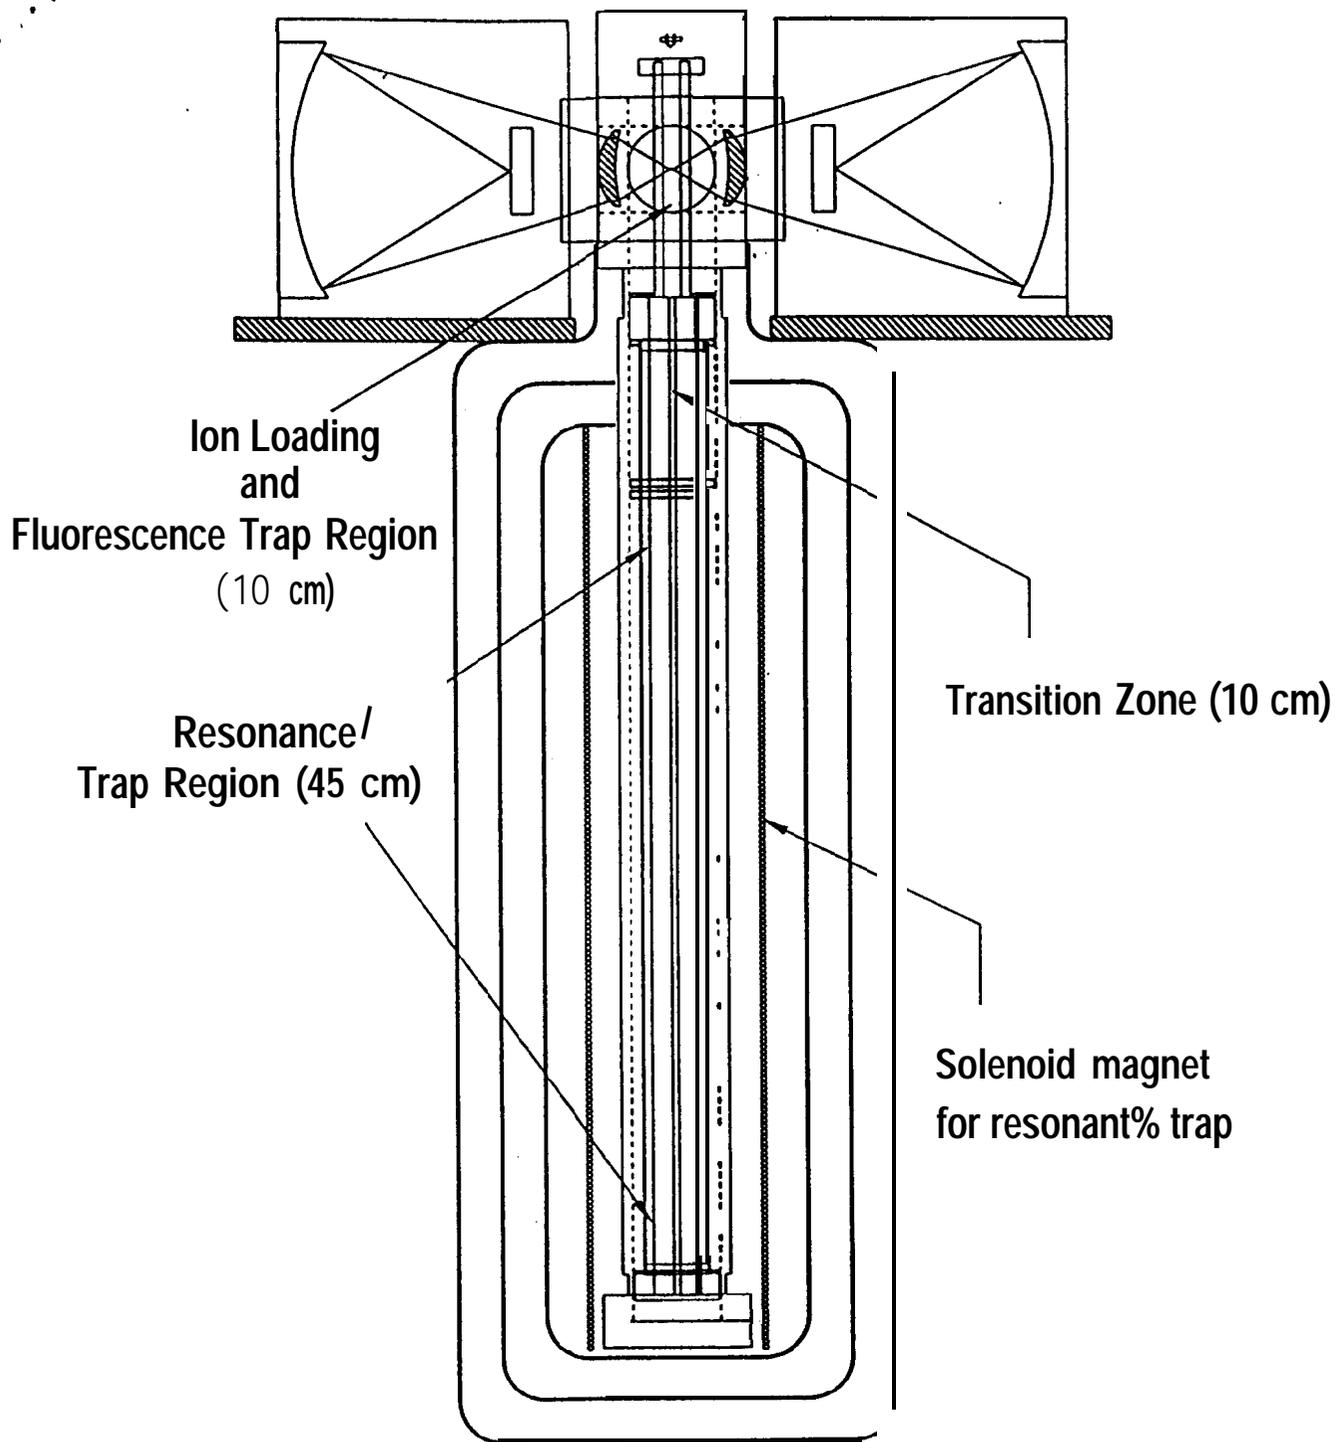


Figure 5: A scaled representation of the new “shuttle” trap incorporated into an existing LITS vacuum and **optical** system. The microwave resonance region is seven **times** longer than in the original LITS to reduce sensitivity to the Second Order Doppler shift.